



## Relative Human Mitochondrial DNA Copy Number Quantification qPCR Assay Kit (RHMQ)

Catalog #8938  
100 reactions

### Product Description

Mitochondrial DNA (mtDNA) is circular, multicopy genome DNA located in mitochondrion, a cellular organelle that plays a key role in energy production of the cell. The capacity for energy production in a cell depends on both mtDNA integrity and copy number. Substantial evidence suggests that alterations in mtDNA copy number have been correlated with aging and various age-related disorders, such as cancer, diabetes and neurodegenerative diseases.

ScienCell's Relative Human Mitochondrial DNA Copy Number Quantification qPCR Assay Kit (RHMQ) is designed to directly compare the average mtDNA copy number of the samples. The mtDNA primer set recognizes and amplifies one of the most conserved regions on human mtDNA and will not amplify any off-target sequence on nuclear genomic DNA. The single copy reference (SCR) primer set recognizes and amplifies a 100 bp-long region on human chromosome 17 and serves as reference for data normalization. The carefully designed primers ensure: (i) high efficiency for trustworthy quantification; and (ii) no non-specific amplification. Each primer set has been validated by qPCR with melt curve analysis and gel electrophoresis for amplification specificity and by template serial dilution for amplification efficiency. The 2X GoldNStart TaqGreen qPCR Master Mix (Cat #MB6018a-1) is a SYBR<sup>®</sup>Green dye-based qPCR master mix with a “hot-start” property. It contains SYBR<sup>®</sup>Green, dNTPs, Taq DNA polymerase, and an inert gold-color loading indicator in a single tube. The “hot-start” property achieved through ScienCell’s unique chemically modified Taq DNA polymerase provides maximal inhibition of primer dimer formation. The advanced buffer formulation provides superior specificity and efficiency with a wide linear dynamic range. The inert gold-color loading indicator allows for better visualization and tracking of sample loading in qPCR plates or tubes.

### Kit Components

Cat #	Component	Quantity	Storage
MB6018a-1	2X GoldNStart TaqGreen qPCR master mix, 1 mL	2 vials	-20°C
8938a	Human mtDNA primer set, lyophilized	1 vial	-20°C
8938b	Single copy reference (SCR) primer set, lyophilized	1 vial	-20°C
8938c	Nuclease-free H <sub>2</sub> O	4 mL	4°C

### Additional Materials Required (Materials Not Included in Kit)

Component	Recommended
DNA isolation kit	SpeedDNA Isolation Kit (ScienCell, Cat #MB6918)
genomic DNA template	Customers' samples
qPCR plate or tube	

**Quality Control**

The specificity of the primer sets is validated by qPCR with melt curve analysis. The PCR products are analyzed by gel electrophoresis. The efficiency of the primer sets is validated by template serial dilution (See **Appendices 1 and 2**).

**Product Use**

RHMQ is for research use only. It is not approved for human or animal use, or for application in clinical or *in vitro* diagnostic procedures.

**Shipping and Storage**

The product is shipped on dry ice. Upon receipt, store the GoldNStart TaqGreen qPCR master mix (Cat #MB6018a-1) in the dark at -20°C in a manual defrost freezer, the primers (Cat #8938a and 8938b) at -20°C in a manual defrost freezer, and the nuclease-free H<sub>2</sub>O (Cat #8938c) at 4°C. Once thawed, do NOT refreeze GoldNStart TaqGreen qPCR master mix (Cat #MB6018a-1), and keep in the dark at 4°C or on ice at all times.

## Procedures

**Important:** *Only use polymerases with hot-start capability to prevent possible primer-dimer formation. Only use nuclease-free reagents in PCR amplification.*

1. Prior to use, allow vials (Cat #8938a and #8938b) to warm to room temperature.
2. Centrifuge the vials at 1,500x g for 1 minute.
3. Add 200  $\mu$ l nuclease-free H<sub>2</sub>O (Cat #8938c) to mtDNA primer set (lyophilized, Cat #8938a) to make mtDNA primer stock solution. Aliquot as needed. Store at -20°C in a manual defrost freezer. Avoid repeated freeze-and-thaw cycles.
4. Add 200  $\mu$ l nuclease-free H<sub>2</sub>O (Cat #8938c) to SCR primer set (lyophilized, Cat #8938b) to make SCR primer stock solution. Aliquot as needed. Store at -20°C in a manual defrost freezer. Avoid repeated freeze-and-thaw cycles.
5. For each genomic DNA sample, prepare two qPCR reactions, one with mtDNA primer stock solution, and one with SCR primer stock solution. Prepare 20  $\mu$ l qPCR reactions for one well as shown in Table 1.

**Table 1.**

Genomic DNA template (0.5 – 5 ng/ $\mu$ l)	1 $\mu$ l
Primer stock solution (mtDNA or SCR)	2 $\mu$ l
2X GoldNStart TaqGreen qPCR master mix (Cat #MB6018a-1)	10 $\mu$ l
Nuclease-free H <sub>2</sub> O (Cat #8938c)	7 $\mu$ l
<b>Total volume</b>	<b>20 <math>\mu</math>l</b>

6. Seal the qPCR reaction wells. Centrifuge the plates or tubes at 1,500x g for 15 seconds. For maximum reliability, replicates are highly recommended (minimum of 3).
7. Refer to Table 2 for qPCR program setup. The 2X GoldNStart TaqGreen qPCR master mix (Cat #MB6018a-1) contains SYBR<sup>®</sup>Green as the reporter dye and does not contain a ROX passive reference dye. If the qPCR instrument being used has a "ROX passive reference dye" option, please deselect this option.


**Note:** The primary factors that determine optimal annealing temperature are the primer length and primer composition. Based on the properties of mtDNA and SCR primer sets (Cat #8938a and #8938b), we highly recommend an annealing temperature of 52°C as shown in Table 2:

**Table 2.**


Step	Temperature	Time	Number of cycles
Initial denaturation	95°C	10 min	1
Denaturation	95°C	20 sec	32
Annealing	52°C	20 sec	
Extension	72°C	45 sec	

Data acquisition	Plate read		
<i>Optional</i>	<i>Melting curve analysis</i>		1
Hold	20°C	Indefinite	1

**Figure 1.** A typical amplification curve showing the amplification of a qPCR product.

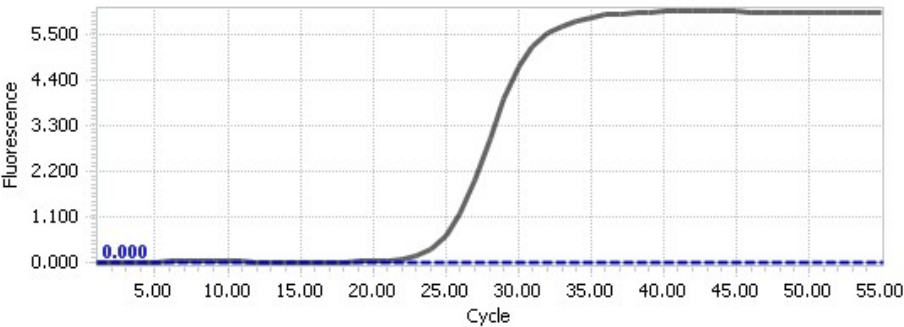

**Figure 2.** A typical melting peak of a qPCR product.

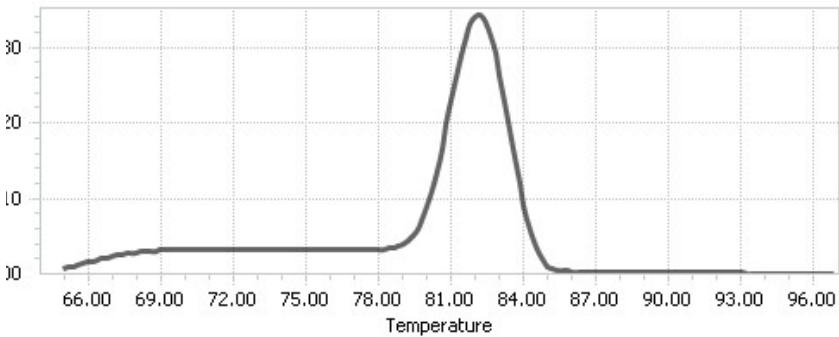

### **Quantification Method: Comparative $\Delta\Delta Cq$ (Quantification Cycle Value) Method**

---

**Note:** Please refer to your qPCR instrument's data analysis software for data analysis. The method provided here serves as guidance for quick manual calculations.

1. For mtDNA,  $\Delta Cq$  (mtDNA) is the quantification cycle number difference of mtDNA between two genomic DNA samples.

$$\Delta Cq (\text{mtDNA}) = Cq (\text{mtDNA, sample 2}) - Cq (\text{mtDNA, sample 1})$$

**Note:** the value of  $\Delta Cq$  (mtDNA) can be positive, 0, or negative.

2. For single copy reference (SCR),  $\Delta Cq$  (SCR) is the quantification cycle number difference of SCR between two genomic DNA samples.

$$\Delta Cq (\text{SCR}) = Cq (\text{SCR, sample 2}) - Cq (\text{SCR, sample 1})$$

**Note:** the value of  $\Delta Cq$  (SCR) can be positive, 0, or negative.

3.  $\Delta\Delta Cq = \Delta Cq (\text{mtDNA}) - \Delta Cq (\text{SCR})$

4. Relative mtDNA copy number of sample 2 to sample 1 (fold) =  $2^{-\Delta\Delta Cq}$

### **Example Calculations: Comparative $\Delta\Delta Cq$ (Quantification Cycle Value) Method**

---

**Table 3.**  $Cq$  (Quantification Cycle) values of mtDNA qPCR (mtDNA) and single copy reference qPCR (SCR) obtained for two genomic DNA samples.

<i>Primer set</i>	<i>Sample 1</i>	<i>Sample 2</i>
mtDNA	16.84	14.16
SCR	26.43	25.20

$$\begin{aligned}\Delta Cq (\text{mtDNA}) &= Cq (\text{mtDNA, sample 2}) - Cq (\text{mtDNA, sample 1}) \\ &= 14.16 - 16.84 \\ &= -2.68\end{aligned}$$


$$\begin{aligned}\Delta Cq (\text{SCR}) &= Cq (\text{SCR, sample 2}) - Cq (\text{SCR, sample 1}) \\ &= 25.20 - 26.43 \\ &= -1.23\end{aligned}$$

$$\begin{aligned}\Delta\Delta Cq &= \Delta Cq (\text{mtDNA}) - \Delta Cq (\text{SCR}) \\ &= -2.68 - (-1.23) \\ &= -1.45\end{aligned}$$

$$\begin{aligned}\text{Relative mtDNA copy number of sample 2 to sample 1 (fold)} &= 2^{-\Delta\Delta C_q} \\ &= 2^{1.45} \\ &= 2.73\end{aligned}$$


***Example Conclusions:*** The average mtDNA copy number of sample 2 is 2.73 fold greater than that of sample 1.

Appendix 1: Quality assessment of mtDNA primer set

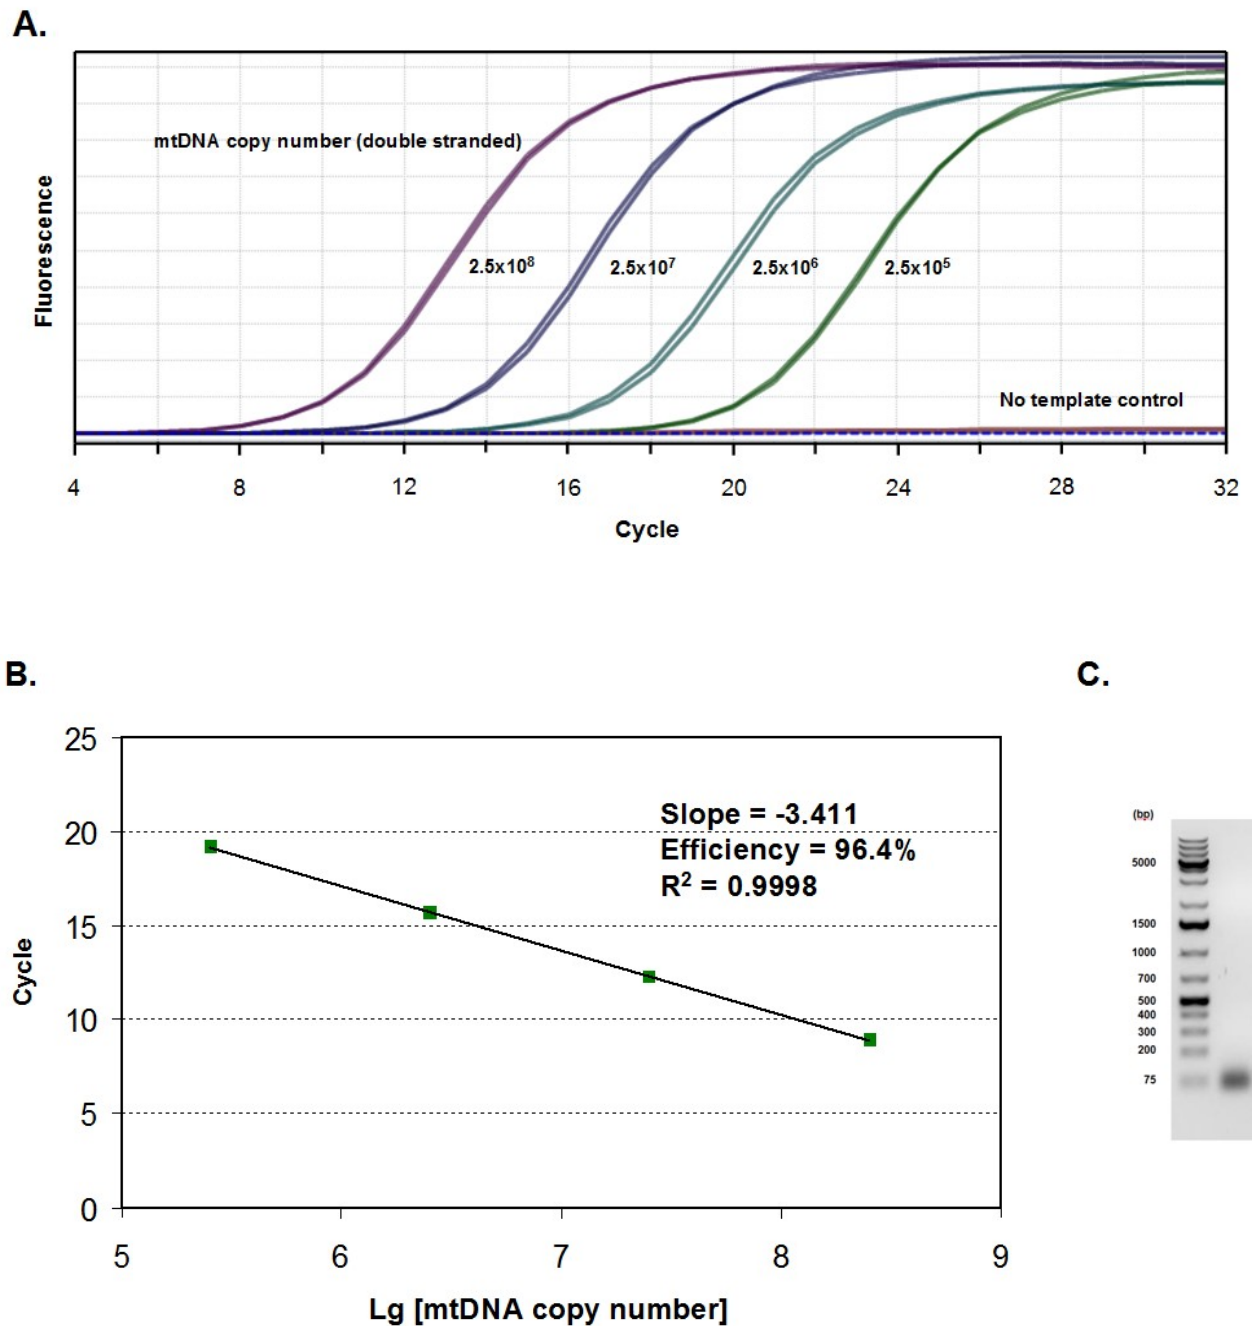

**Figure 3. Quality assessment of mtDNA primer set.** (A) qPCR amplification curves using serially diluted mtDNA template. (B) Derivation of qPCR efficiency of mtDNA primer set. (C) Separation of mtDNA qPCR product by gel electrophoresis.

Appendix 2: Quality assessment of Single copy reference (SCR) primer set

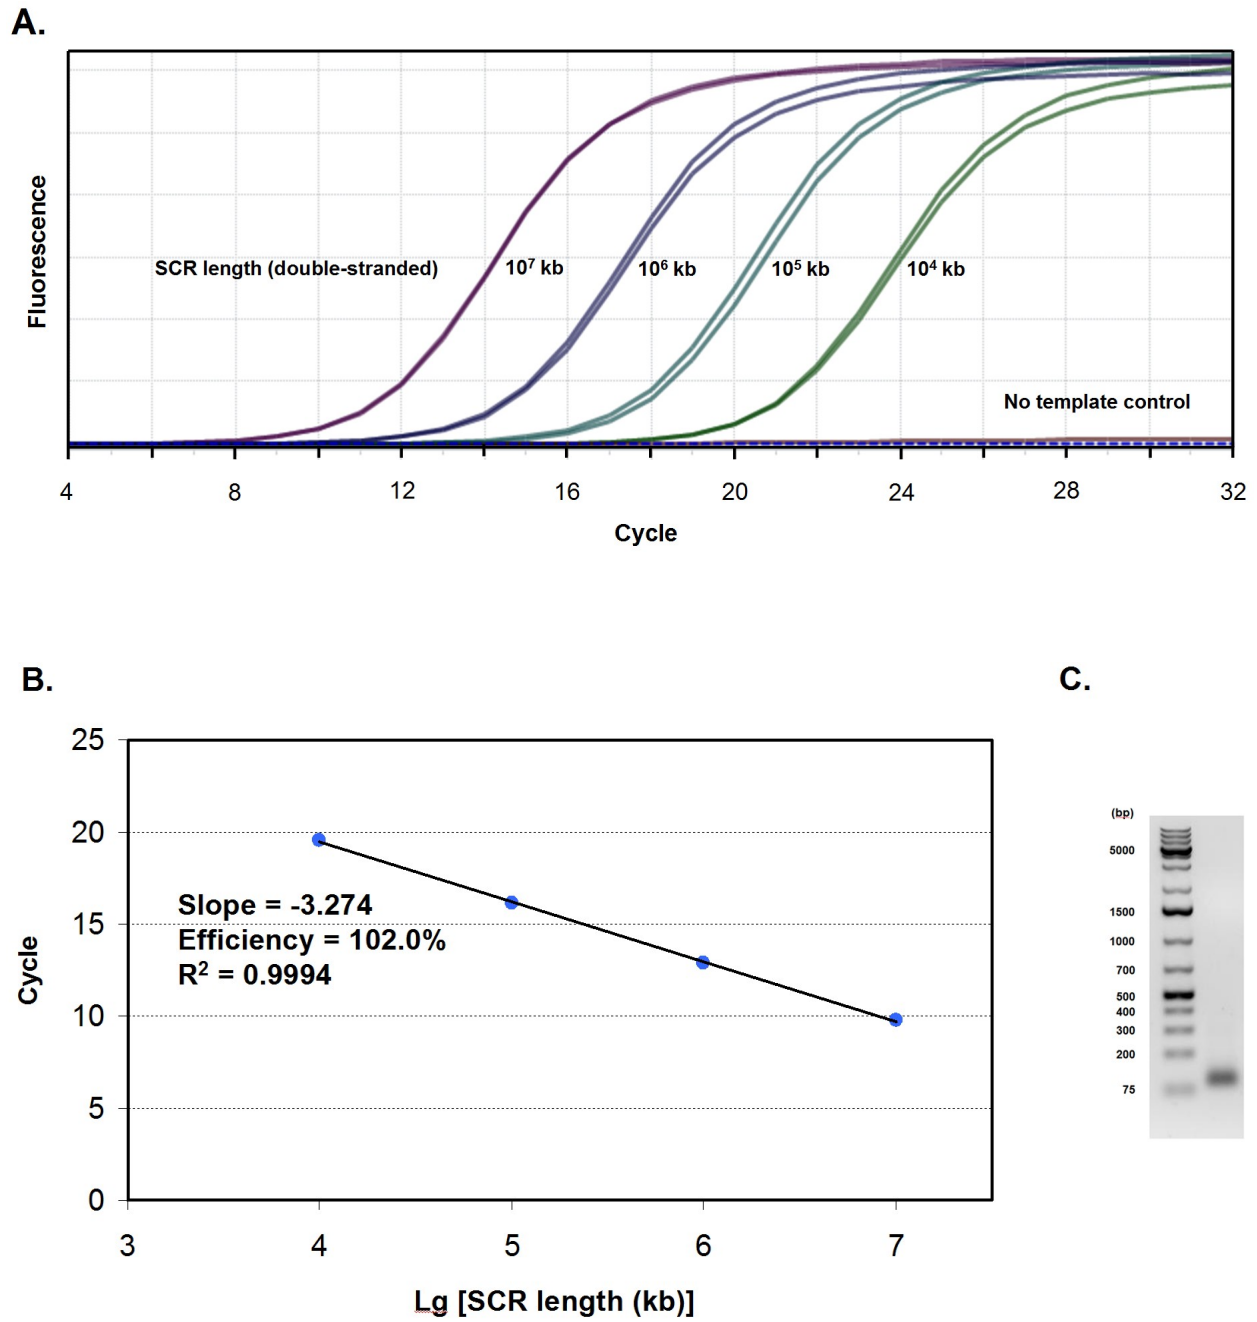

**Figure 4. Quality assessment of Single copy reference (SCR) primer set. (A)** qPCR amplification curves using serially diluted SCR template. **(B)** Derivation of qPCR efficiency of SCR primer set. **(C)** Separation of SCR qPCR product by gel electrophoresis.